



G-Lock

DUODENOSCOPE ED-580XT

FUJIFILM
Value from Innovation




FOR EFFICIENT ERCP PROCEDURES

VIDEO DUODENOSCOPE **ED-580XT**



ERCP (Endoscopic retrograde cholangiopancreatography) uses a combination of endoscopy and fluoroscopy to diagnose and treat the biliary or pancreatic ductal system and requires a high level of expertise from the endoscopist.

The new Fujifilm video duodenoscope is designed to support quality and efficiency and utilises a new G-Lock elevator. A unique distal attachment cap allows easy, fast and efficient cleaning. The ED-580XT is made to support you during your most complex procedures.

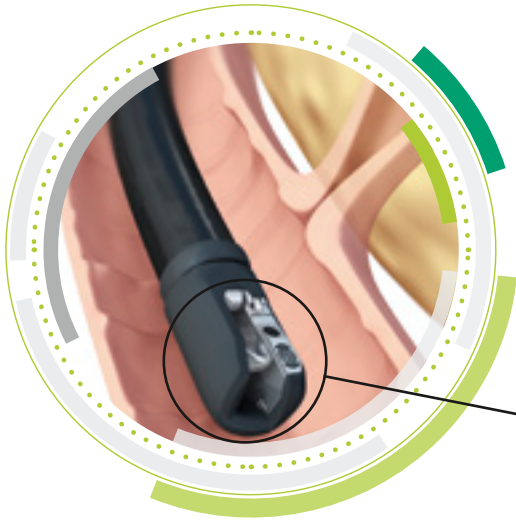

G-Lock

Improved treatment capability





FOR EFFICIENT ERCP PROCEDURES

IMPROVED WIRE LOCKING G-LOCK AND GREATER ELEVATION FORCE



IMPROVED TREATMENT CAPABILITY

Incorporated into the distal tip of the ED-580XT, the G-Lock contains the forceps elevator and the contact section, enabling the guidewire to be simply and securely fixed into position by using the forceps elevator. In addition, the specially designed round shaped forceps elevator reduces the risk of guidewire damage. The inner tube of the instrument channels uses an optimised material to enable a device to be inserted smoothly, supporting rapid device exchange. Designed to work in harmony with the endoscopist, the new G-Lock and low friction instrument channel support efficiency and ease of use during ERCP procedures.

INCREASED ANGLE OF ENDOTHERAPY DEVICES

The forceps elevator design increases the maximum angle that endotherapy devices can be introduced. Movement of the elevator lever at the control body of the duodenoscope translates accurately to the distal tip, allowing for very precise positioning of instruments.



Case image of improved elevation force



G-Lock



ADVANCED MANOEUVRABILITY

ADVANCED FORCE TRANSMISSION

The flexible portion is designed to transmit the pushing, pulling and rotating movements from the hand to the distal end of the endoscope, providing enhanced manoeuvrability inside the digestive tract.

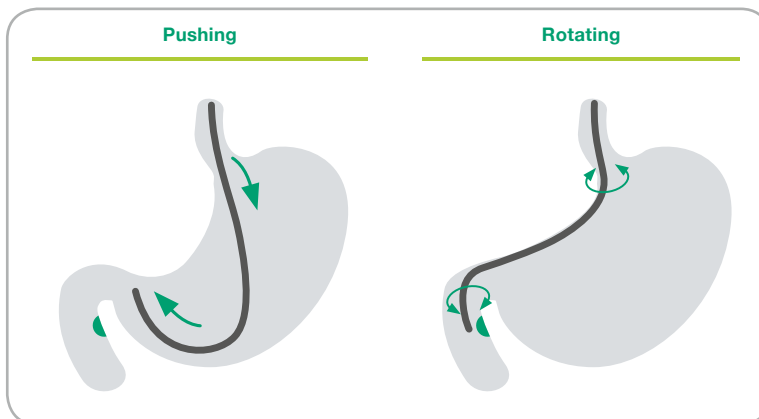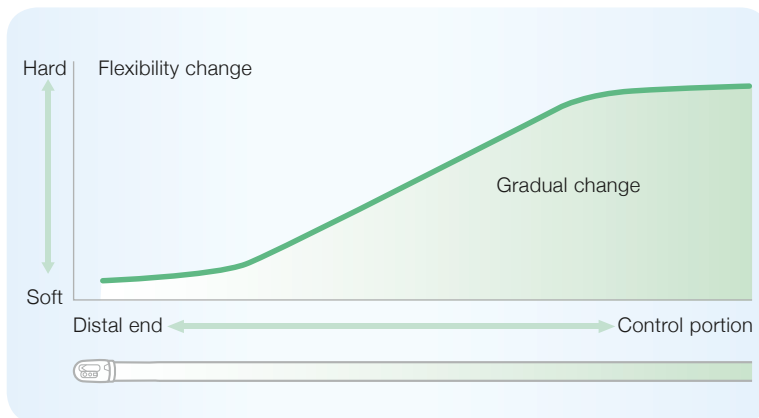

INTUITIVE OPERATION


The G7 control portion has a rounded surface design to fit in the hand, and its layout makes intuitive operation possible.





FOR EFFICIENT ERCP PROCEDURES

EASY AND EFFECTIVE DISTAL END CLEANING



**EASIER
BRUSHING
ACCESS -
EASIER
CLEANING**

The single-use distal end cap permits easier brushing access to the distal end of the endoscope. In addition, the elevator mechanism is sealed to allow easier cleaning.

ATTACHMENT AND DETACHMENT OF DISTAL END CAP

ATTACHMENT



Cover the distal end cap until the installation groove of the distal end is hidden completely.



Make sure that the distal end cap is attached tightly by pulling it straight.

DETACHMENT



Lift up a portion of distal end cap near the instrument channel outlet.




While turning the portion counterclockwise, pull it straight out.

SPECIFICATIONS & ACCESSORIES

NEW DUODENOSCOPE **ED-580XT**



Viewing direction	95° (retro-viewing 5°)
Field of view	100°
Observation range	4–60 mm
Distal end diameter	13.1 mm
Bending capability	Up 120° / Down 90° Left 90° / Right 110°
Working length	1,250 mm
Total length	1,550 mm
Insertion tube diameter	11.3 mm
Minimum diameter of instrument channel	4.2 mm

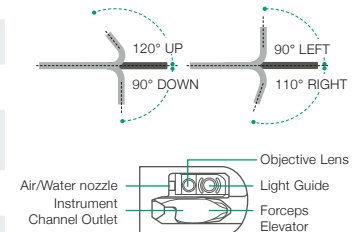

SUPER CCD TECHNOLOGY

The Super CCD and high performance optical system ensures high quality images. It provides brilliant images which can facilitate procedures for detection and treatment of lesions.



FICE TECHNOLOGY

FICE can enhance slight colour differences such as vascular and mucosal patterns without tissue staining. The procedure digitally selects three wavelengths of light and displays reconstructed images.



HD TECHNOLOGY

Combine equipment displaying this logo to ensure that you view HDTV images on your monitor.



SB-605

Suction Valve



AW-603

Air/Water Valve



AW-604G

Gas/Water Valve



DC-07D

Distal End Cap



WB11003DV

Disposable Cleaning Brushes



WB7025DC

Disposable Cleaning Brushes



WB1318DE

**ADVANCING DEEPER INSIGHTS
IN ENDOSCOPY**

FUJIFILM

FUJIFILM Europe GmbH

Heesenstr. 31, 40549 Düsseldorf, Germany
Tel.: +49 211-50 89 0, Fax: +49 211-50 89 8700
www.fujifilm.eu, endoscopy_eu@fujifilm.com